

AB Tip İnceleme Sertifikası EU Type-Examination Certificate

Belge No / Certificate No

: 217-21-01

Belgelendirme Tarihi - Bir Sonraki Belge Tarihi /

Certification Date / Certificate Validity Date

: 09.04.2021-09.04.2026

Belge Geçerlilik Tarihi / Document Validity Period: 5 yıl / 5 years

Firma Unvanı ve Adresi /

Company Name and Address

: BYM SAĞLIK MEDİKAL ENERJİ SAN.

VE TİC. A.Ş.

Cevizli Mah. 1236 Sk. Zorlu Apt. No: 2 İç

Kapı No: 7 Çankaya/ ANKARA

Ürün Adı /Modeller / Product Name / Models

Direktifi / Directive

Modülü/Kategori / Module / Category

: 2016/425 REGULATION

: B MODÜLÜ/ KATEGORİ III MODULE B / CATEGORY III

: MNA M-2021-00607

Test Rapor No/ları / Test Report No Ürün Tipi / Product Type:

 EN 149:2001+ A1:2009 Solunumla ilgili koruyucu cihazlar - Parçacıklara karşı koruma amaçlı filtreli yarım maskeler/ Respiratory protective devices - Filtering half masks to protect against particles

Ürünün Malzeme Bilgisi / Product Material Information: BYM-001 model ürünleri kumaş, elastik kayış, burun klipsi, filtre katmanı kullanılarak imal edilmiştir./ BYM-001 model products are manufactured using fabric, elastic strap, nose clip, filter layer.

Volkan AKIN 09.04.2021 Karar Verici / Approver

Okan AKEL 09.04.2021 Şirket Müdürü / General manager










ATTACHMENTS (217-21-01)

To certify the PPE product at Category III level, C2 or D module is accompanied by applying one of the conformity assessment methods along with the EU Type Examination (Module B).

Model: BYM-001

PPE SPECIFICATION	PERFORMANCE LEVELS
Classification	FFP2
Reusable / Single Shift Use	NR


PPE produced as a single unit to fit an individual user, all the necessary instructions for manufacturing such PPE on the basis of the approved basic model:

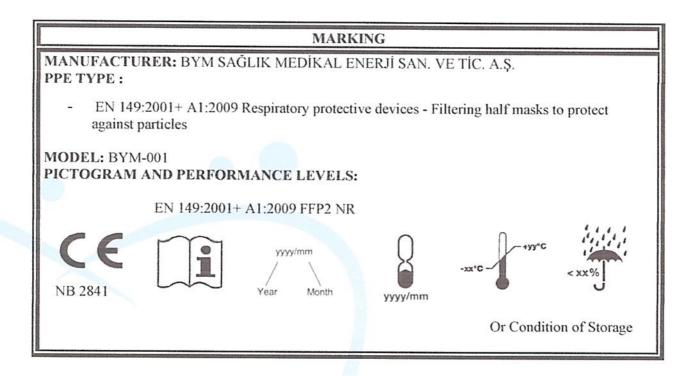

MNA LABORATORIES SAN. TIC. LTD. \$TI declares that the above-mentioned product meets the requirements of the directive according to the EU Directive 2016/425, the safety of the product is covered by the conditions and use specified in this certificate and in the technical file.



ATTACHMENTS (217-21-01)

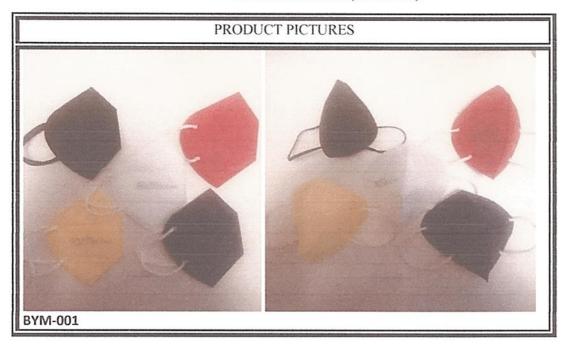

DOCUMENTS IN THE TECHNICAL FILE

- Basic Health Safety Requirements
- Risk Assessment
- Test Reports
- Technical Report



TECHNICAL EVALUATION REPORT (217-21-01)

Report No : 217-21-01

Report Date : 09.04.2021

Application No : 217-21-01

1. COMPANY INFORMATION:

BYM SAĞLIK MEDİKAL ENERJİ SAN. VE TİC. A.Ş.

Cevizli Mah. 1236 Sk. Zorlu Apt. No: 2 İç Kapı No: 7 Çankaya/ ANKARA


2. PPE INFORMATION:

Disposable and non-sterile half mask made of particulate protection fitler material.

3. PPE TYPE IDENTIFICATION

EN 149:2001+A1:2009 Respiratory protective devices – Filtering half masks to protect against particles - Requirements, testing, marking

4. PPE PICTURES

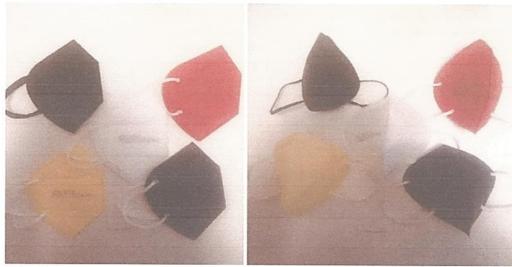

BYM-001

5. PPE DIMENSIONS:

BYM-001 model has been found to be produced using standart sizes.

6. PPE PRODUCT MATERIAL INFORMATION:

The product is made of elastic strap, nonwoven fabric on the outer and inner layers and fitler material on the middle layer.

7. ESSENTIAL HEALTH AND SAFETY REQUIREMENTS

- A visual inspection was made according to EN 149:2001 +A1:2009 for ergonomics.
- Protection levels and degrees are defined by the manufacturer.
- Suitable construction materials were determined by visual inspection according to EN 149:2001 +A1:2009.



TECHNICAL EVALUATION REPORT (217-21-01)

8. ANALYSIS AND EVALUATIONS: EN 149:2001 +A1:2009

TESTS	PARAMETER	PERFORMANCE LEVELS			RESULTS	PERFORMANCE LEVELS	EVALUATION
		FFP1	FFP2	FFP3			
Part 7.3 Visual inspection	Shall also the marking and the information supplied by the manufacturer				Appropriate	-	PASS
Banned Azo Dyes	< 30 mg/kg			< 5 mg/kg	-	PASS	
Part 7.4 Packaging	Particle filtering half mask shall be offered for sale packaged in such a way that they are protected against mechanical damage and contamination before use.			Appropriate	-	PASS	
Part 7.5 Material	When conditioned in accordance 8.3.1 & 8.3.2 the particle filter half mask shall not collapse.				Appropriate	-	PASS
Part 7.6 Cleaning and disinfecting	After cleaning and disinfecting the re-usable			Not applicable	-	Not applicable	
Part 7.7 Practical performance	T	to negative comments should be made by the test subject regarding any of the criteria valuated.			Appropriate	-	PASS
Part 7.8 Finish of parts	Parts of the device likely to come into contact with the wearer shall have no sharp edge or burrs.				Appropriate	-	PASS

TESTS	PARAMETER	PERFORMANCE LEVELS			RESULTS	PERFORMANCE LEVELS	EVALUATION
		FFP1	FFP2	FFP3	1		
Part 7.9.1 Total inward leakage	At least 46 out of the 50 individual exercise result	<25	<11	<5	See the table below	FFP2	PASS
	At least 8 out of the 10 individual wearer arithmetic means	<22	<8	<2	See the table below	FFP2	PASS

Total Inward Leakage (%)										
	Exercise 1	Exercise 2	Exercise 3	Exercise 4	Exercise 5	Average				
Subject 1 (As recieved)	7.4	8.6	8.0	8.5	6.8	7.9				
Subject 2 (As recieved)	8.0	5.6	6.1	6.8	6.7	6.6				
Subject 3 (As recieved)	7.7	8.9	7.4	8.6	8.0	8.1				
Subject 4 (As recieved)	7.6	8.3	8.1	8.6	8.9	8.3				
Subject 5 (As recieved)	7.4	8.6	8.0	5.7	7.5	7.4				
Subject 6 (After temperature conditioning)	7.7	8.0	6.2	6.8	9.0	7.5				
Subject 7 (After temperature conditioning)	7.4	7.4	8.6	8.0	7.5	7.8				
Subject 8 (After temperature conditioning)	7.4	8.6	8.0	8.0	7.7	7.9				
Subject 9 (After temperature conditioning)	8.6	8.0	6.2	8.5	8.0	7.9				
Subject 10 (After temperature conditioning)	6.2	8.5	5.7	7.5	8.5	7.3				



MNA LABORATUVARLARI SAN. TİC, LTD, ŞTİ.

MNA LABORATUVARLARI

TECHNICAL EVALUATION REPORT (217-21-01)

TESTS PARAMETER	PARAMETER	PERFORMANCE LEVELS			RESULTS	PERFORMANCE	EVALUATION
	FFP1	FFP2	FFP3		LEVELS		
Part 7.9.2 Penetration of filter	Sodium chloride, 95 L/min %, max	% 20	%6	% 1	See the table below	FFP2	PASS
material	Paraffin oil, 95 L/min %, max	% 20	% 6	%1	See the table below	FFP2	PASS

Penetration of filter material	Sodium Chloride (%)	Paraffin Oil (%)	
As recieved	3.9	4.2	
As recieved	4.2	4.5	
As recieved	4.2	4.4	
After the simulated wearing treatment	4.2	4.4	
After the simulated wearing treatment	4.1	4.6	
After the simulated wearing treatment	4.2	4.5	
Mechanical strength and temperature conditioning	5.7	5.2	
Mechanical strength and temperature conditioning	5.5	5.8	
Mechanical strength and temperature conditioning	5.3	5.5	

TESTS PARAMETER	PARAMETER PERFORMANCE LEVELS			RESULTS	PERFORMANCE	EVALUATION	
	FFP1	FFP2	FFP3		LEVELS		
Part 7.10 Compatibility with skin	Materials shall not cause irritation or a health		Appropriate	=	PASS		
Part 7.11 Flammibility	Mask shall not burn for more than 5 s	or not to	continu	e to burn	Flame not seen	-	PASS
Part 7.12 Carbondioxide content of the inhalation air	Shall not exceed an	average o	f % 1		0,86 0,80 0,85	-	PASS
Part 7.13 Head harness	It can be donned and removed easily				Appropriate	-	PASS
Part 7.14 Field of vision	The field of vision s performance test.	hall accep	table in	practical	Appropriate	-	PASS
Part 7.15 Exhalation valve(s)	It shall withstand axially a tensile force of 10 N apply for 10 s. If fitted, shall continue to operate correctly after a continuous exhalation flow of 300 L/min over a period of 30 s.				Not applicable	-	Not applicable



TECHNICAL EVALUATION REPORT (217-21-01)

TESTS PARAMETER	PARAMETER	PERFORMANCE LEVELS			RESULTS	PERFORMANCE	EVALUATION
	FFP1	FFP2	FFP3		LEVELS		
Part 7.16 Breathing	Inhalation 30L/min	0,6 mbar	0,7 mbar	1,0 mbar	See the table below	FFP2	PASS
Resistance Inhalation 95L,	Inhalation 95L/min	2,1 mbar	2,4 mbar	3,0 mbar	See the table below	FFP2	PASS
	Exhalation 160L/min	3,0 mbar	3,0 mbar	3,0 mbar	See the table below	FFP2	PASS

Breathing Resistance (mbar)	Inhalation 30L/min	Inhalation 95L/min
As recieved	0,6	2,2
As recieved	0,6	2,2
As recieved	0,5	2,3
After temperature conditioning	0,5	2,3
After temperature conditioning	0,6	2,3
After temperature conditioning	0,5	2,2
After the simulated wearing treatment	0,5	2,3
After the simulated wearing treatment	0,6	2,3
After the simulated wearing treatment	0,6	2,3
After the flow conditioning	-	-
After the flow conditioning	-	-
After the flow conditioning	-	-

Breathing Resistance 160L/min (mbar)	Facing directly ahead	Facing vertically upwards	Facing vertically downwards	Lying on the left side	Lying on the right side
As recieved	2,8	2,8	2,8	2,7	2,8
As recieved	2,7	2,8	2,8	2,7	2,8
As recieved	2,7	2,8	2,8	2,7	2,8
After temperature conditioning	2,7	2,8	2,8	2,8	2,8
After temperature conditioning	2,8	2,8	2,8	2,8	2,8
After temperature conditioning	2,8	2,8	2,8	2,8	2,8
After the simulated wearing treatment	2,8	2,8	2,7	2,8	2,8
After the simulated wearing treatment	2,8	2,8	2,7	2,8	2,8
After the simulated wearing treatment	2,8	2,8	2,8	2,8	2,8
After the flow conditioning	-	-	-	-	-
After the flow conditioning	-	-	-	-	-
After the flow conditioning	-	-	-	-	-



TECHNICAL EVALUATION REPORT (217-21-01)

TESTS PARAMETER	PARAMETER	PERFC LEVEL	RMANO S	Œ	RESULTS	PERFORMANCE LEVELS	EVALUATION
		FFP1	FFP2	FFP3			
Part 7.17 Clogging	After clogging the inhalation resistances shall not exceed. (valved)	4 mbar	5 mbar	7 mbar	Not applicable	-	Not applicable
	The exhalation resist 3 mbar at 160 L/ (valved)				Not applicable	-	Not applicable
		Not applicable	-	Not applicable			
Part 7.18 Demountable part	All demountable par readily connected possible by hand.		itted) sl ecured		Not applicable	-	Not applicable

9. DECISION

Analysis and examinations BYM-001 model coded personal protective equipment; Respiratory Protective Devices EN 149:2001 +A1:2009- Filtered Half Masks for Protection Against Particles - Properties, Experiments and Marking standards are evaluated. It is recommended to be certified at the performance levels specified as a result of technical evaluations.

10. ATTACHMENTS

- Basic Health Safety Requirements
- Risk Assessment
- User Instruction

CONTROLLER

: VOLKAN AKIN

SING

DATE

6000 7011